


## 1. Materials


Kit	ExiPrep™ Bacteria Genomic DNA Kit
Instrument type	ExiPrep™16 Plus
Sample type	Urine
Sample amount	Up to 15ml
Protocol ID number	108
Elution volume	100µl

## 2. Experimental Procedure

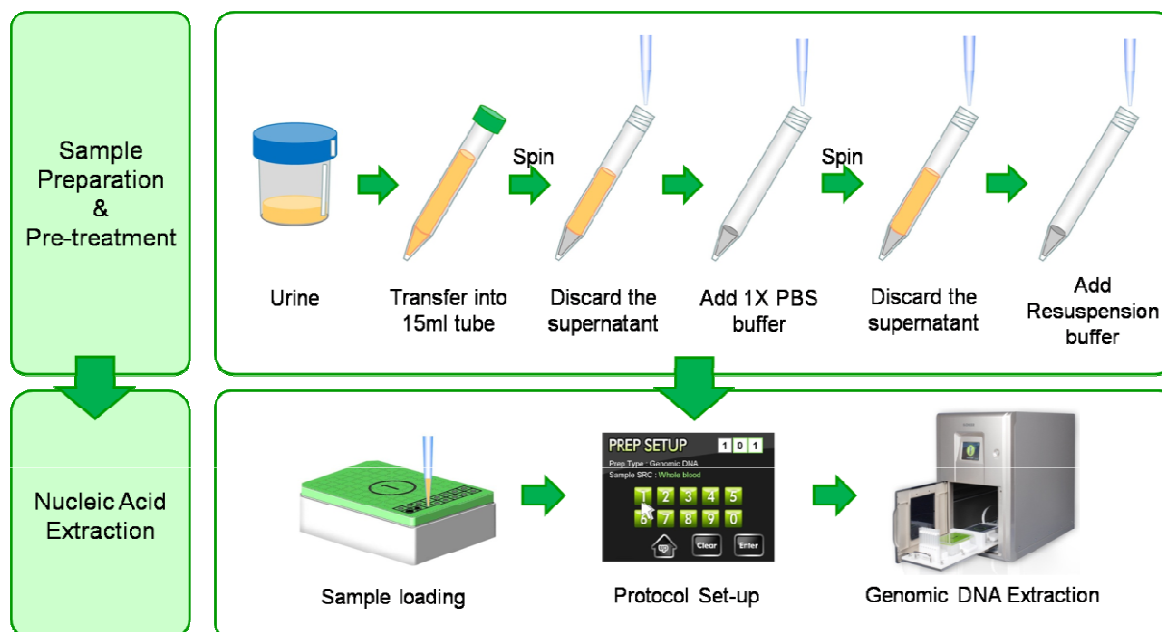

## 3. Experimental Results

### - Real time PCR result

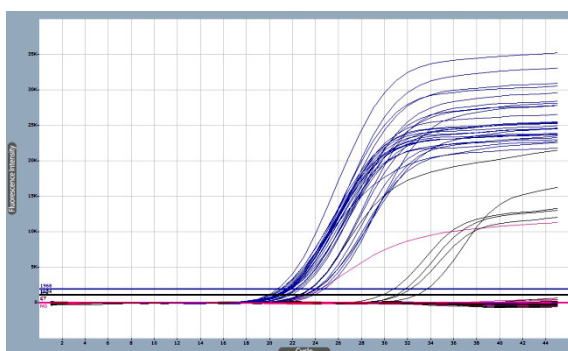

Real-time PCR results using *AccuPower*® CT & NG Real-time PCR Kit(CNM-1111, Bioneer) and run on *Exicycler*™ 96 Real-Time PCR System(Cat. No. : A-2060) from genomic DNA extracted from urine samples.