


1. Materials


| | |
|--------------------|-----------------------------|
| Kit | ExiPrep™ Viral DNA/ RNA Kit |
| Instrument type | ExiPrep™16 Plus |
| Sample type | Swab |
| Sample amount | 1 ea |
| Protocol ID number | 518 |
| Elution volume | 50 µℓ |

2. Experimental Procedure

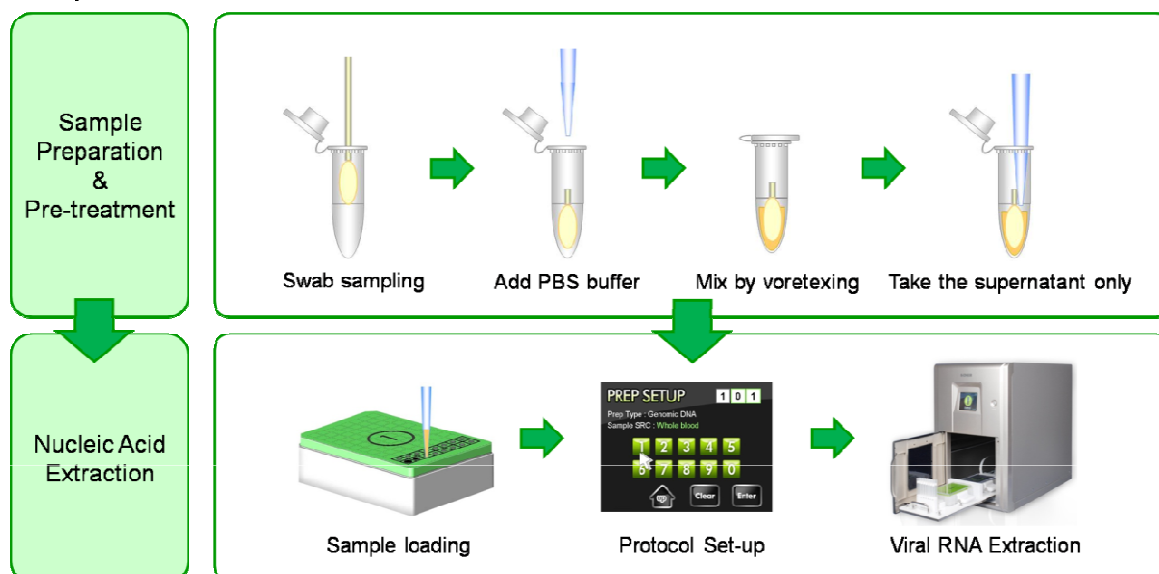

3. Experimental Results

- Real time PCR result

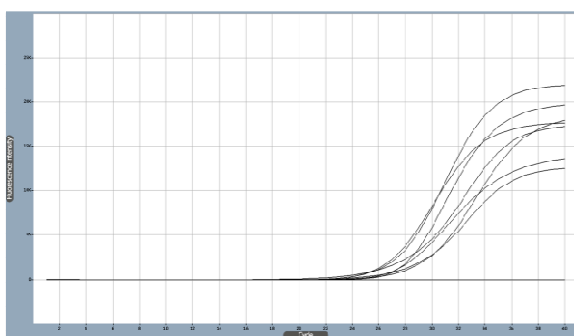

Real-time RT-PCR results using *AccuPower*® new Inf A(H1N1) & Inf A Real-time PCR Kit(SIA-1111, Bioneer) and run on *Exicycler*™ 96 Real-Time PCR System(Cat. No.: A-2060) from viral RNA extracted from swab samples.