


ExiProgen™ EC-Disulfide Protein Synthesis Kit (Cat. No. K-7330)

Step I Preparation of Template DNA

- 1) Prepare the 'Template DNA' for protein expression.
(Note I) The 'Template DNA' must contain the following: T7 Promoter, Ribosome binding site (RBS) Target gene (with His-tag), and T7 terminator.
(Note II) Use **1 µg/kb** (insert size of DNA) of plasmid DNA (Purity: $A_{260/280} > 1.7$, $A_{260/230} > 1.5$).

Step II Preparation of Experiment

- 1) Take out the 'Cartridge ②' from **Box ②**. Thaw them at room temperature.
- 2) Take out 'E. coli extract', 'Master Mix', 'DEPC DW' and 'Storage Buffer' from **Box ②** and thaw them on ice. Take out 'Cartridge ①', 'Disposable Filter Tip', and 'Protection Cover' from **Box ①**.
(Note) Make sure that all the solutions are completely thawed. It takes about 2 hours.
- 3) Prepare the 'Reaction Block' (ExiProgen™ accessory).
- 4) Take out twice as many 'Dialysis Tube' as the number of samples from **Box ①**.
- 5) Remove the solution in the 'Dialysis Tube' and rinse inside and out using squeeze bottle with sterile distilled water.
(Note) The solution in the 'Dialysis Tube' is 20%(v/v) ethanol.
- 6) Install the 'Dialysis Tube' on the 'Reaction Block', as shown in the diagram.



- 7) Remove water in the 'Dialysis Tubes' and prepare expression solution as shown in the table.

The expression solution should be loaded at the 'Dialysis Tube' in **row A** (Protein expression section). Fill **500 µl** of sterile distilled water in the 'Dialysis Tube' on **row B** (Dialysis section).


* Composition of Expression Solution

	Sample	Positive control DNA (Optional)
Template DNA	X µl	2 µl
E. coli extract	120 µl	120 µl
Master Mix	210 µl	210 µl
DEPC DW	(120-X) µl	118 µl
Total volume	450 µl	450 µl



- 8) Place the 'Protection Cover' on the 'Reaction Block'.
- 9) Punch holes in the sealing films of 'Cartridge ①, ②'.
- 10) Add 1ml of 'Storage Buffer' G1-I2 rows of 'Cartridge ②'.

(Note) The number of columns punched should match with the sample number.

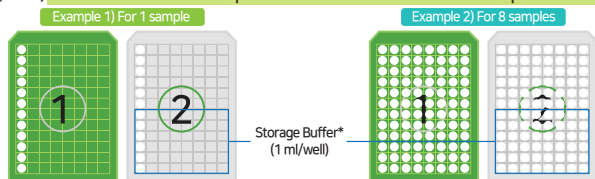

* Composition of Storage Buffer


- 50 mM Tris-HCl, 100 mM NaCl, 1 mM DTT, 0.05%(v/v) Na₂S₂O₃, 50%(v/v) glycerol, pH 7.6.

Step III Protein Synthesis with ExiProgen™

- 1) Turn on the ExiProgen™ and tap 'Press to Start' button.
Wait until the [MENU] screen appears.

ExiProgen™ EC-Disulfide Protein Synthesis Kit (Cat. No. K-7330)

- Open the door of ExiProgen™ and pull out the baseplate.
- Load 'Cartridge ①', 'Waste Tray', and 'Reaction Block'.
Follow in order: 'Cartridge ②' → 'Cartridge ①' → 'Waste Tray' → 'Reaction Block'.
(Note I) Make sure that the first and second lines of 'Cartridge ②' are firmly fixed on the heating block.
(Note II) There are 'silicon rings' embedded on both sides of the 'Cartridge ①' installation position. Place the left side first, and then the right side.
- Place the 'Disposable Filter Tips' on row B of 'Disposable Tip Rack'.
(Note) Tips should be placed in the same columns with the punched holes of the Cartridges.




- Push the baseplate in until you hear the click sound, then close the door.
- Tap the following: [MENU] 'Start' → [PREP SETUP] '905 (Synthesis_DS)' 'Enter' → [PREP SETUP, Elution Volume] 'OK' → [PREP SETUP, Reaction Temperature] '26°C' 'OK' → [CHECK LIST] 'OK' → [Running Mode] 'RUN'.



- The [Work Completion] screen will appear once the protocol is completed.
It takes approximately 36 hours.
- Purified protein samples in the 'Storage Buffer' can be collected from the 'Dialysis Tube', located at the row B of the 'Reaction Block'.

Step IV Analysis of Sample

A. Position of each sample (in 'Cartridge ②')



- Expression sample**: Samples after expression, but without purification
- Unbound sample**: Samples not bound to Ni-NTA magnetic bead
- 1st washing sample**: Samples after 1st washing step in purification process
- Bead sample**: Used bead samples for purification

B. Sampling for SDS-PAGE analysis

- Prepare loading mixture as shown in the table. Incubate the samples at 95°C for 5-10 min.

	Expression/Unbound/ 1 st washing sample	Purified protein sample	Bead sample
Sample	5 µl	10 µl	15 µl
4X Loading dye	5 µl	5 µl	5 µl
Sterile distilled water	10 µl	5 µl	-
Total volume	20 µl	20 µl	20 µl

(Note) Add 100 µl of sterile distilled water to the well containing the beads for suspension. Proceed with the sampling afterwards.

- Load each sample to wells of SDS-PAGE gel [10 x 8 (cm), 0.75 mm thick, 10-well].
(Note) Expression, Unbound and 1st washing samples: 5 µl/well,
Purified proteins and Bead samples: 10 µl/well

※ For more information, visit our [website \(www.bioneer.com\)](http://www.bioneer.com).